

J-2000

WOOD MOISTURE METER

OPERATION MANUAL



DELMHORST EUROPE

TITANIUMLAAN 100
NL 5221 CK 's-HERTOGENBOSCH
THE NETHERLANDS

info@delmhorst.eu
www.MoistureMetersDelmhorst.com
+31 (0)73 6395080

**ADDENDUM TO MODEL J-2000 OWNERS MANUAL
FOR MODEL J-2000/X**

FOLLOWING ARE CHANGES MADE TO THE STANDARD J-2000:

The model J-2000/X has an expanded moisture content range from 6% to 60%.

All other topics in the standard operating instructions for the J-2000 remain in effect.

TABLE OF CONTENTS

J-2000 Features	4
Before You Begin	5
Button Functions	5
Check Calibration	5
Set Species	5
Species Code Chart	6
Set Temperature	6
Set Temperature Mode	7
Set pin calibration	7
Taking a Reading	7
Information About Your Readings	8
To Check Accumulated Readings	8
To Reset the Meter	8
Pin talk	8
Care of Your Meter	9
Service For Your Meter	9
Warranty	10



This product is covered by EU directive 2002/96/EC (WEEE). For disposal please contact your supplier or local authorities for instructions as to best do so.



J-2000 FEATURES

- Resistance technology recognized world wide as the most accurate method for measuring moisture
- 6% - 40% moisture range
- Digital readout
- Averages up to 100 accumulated readings
- Built-in correction for 48 different species
- Built-in temperature compensation both Fahrenheit and Celsius
- Proven microcontroller circuit for increased reliability and accuracy
- Easy one-hand operation
- Includes (1) 9-Volt Battery
- Includes a sturdy carrying case
- One year warranty
- For 60 years of proven quality, accuracy and service

BEFORE YOU BEGIN

BUTTON FUNCTIONS



(#1) Read Button - Reads the Percent Moisture Content value (%MC), corrected for temperature and species.



(#2) Calibration Check Button - Checks meter calibration. It also displays the average of up to 100 accumulated readings; displays the maximum stored reading; erases the readings.



(#3) Species Button - Sets the species code for the wood you are using. Species are numbered from 1 to 50 and are listed on the **Species Code Chart**. This button also acts as a scroll key, depending on the function.



(#4) Temperature Button - Sets the wood temperature. This button also acts as a scroll key, depending on the function.

CHECK CALIBRATION ✓

Press the calibration check button #2 and read button #1 simultaneously. Meter is in calibration if it displays 12% (+ or - .2).

If you check the calibration and the meter does not display 12% it is likely an indication of a low battery. If this occurs, change the battery immediately. Continued use with a low battery may cause the meter to go out of calibration. If you have a fresh battery and the instrument still does not indicate a proper calibration, return it to DELMHORST for service. See "**Service for Your Meter**" section.

When the battery is removed and then reconnected, the meter displays its software version for one second and then turns itself off. After replacing the battery, you must reset the meter as described in "**Resetting the Meter**" section.

SET SPECIES 🌲

The J-2000 defaults to Species Code # 1 – Douglas Fir. Because the electrical characteristics of different species vary, all species read differently at the same moisture content. For this reason you need to adjust for species. If you are working with a species other than Douglas Fir, set the species code using the species button (#3), and the meter will make the necessary corrections.

- **To change species** press the species button (#3). The meter will display the current species code for one second.
- **To scroll forward** through the species list hold the species button (#3) while the current species code is displayed and scroll to the species number desired.
- **To scroll backward** through the species list, press and release the species button (#3). Within one second, press and hold the temperature button (#4). Continue to hold the temperature button (#4) and the species number will decrease.
- **When scrolling in either direction**, release the button to stop at your desired species.

The J-2000 can be used to test more than just wood. It will also give a relative reading on plywood, OSB, particleboard and MDF or can be fitted with a 26-ES slide hammer for specific applications. Call Delmhorst Europe at +31 736395080 or e-mail info@Delmhorst.eu for information on how to interpret the readings for other materials.

SPECIES CODE CHART

Code	Species	Code	Species
1	Fir, Douglas	25	Magnolia
2	Pine, Southern	26	Mahogany, African (also Khaya)
3	SPF	27	Mahogany, Honduras
4	Alder	28	Mahogany, Philippine
5	Apitong	29	Maple, Hard/Soft
6	Aspen	30	Meranti, Dark Red
7	Ash, White	31	Oak, Red
8	Basswood	32	Oak, White
9	Birch, Merbau	33	Pecan
10	Cedar, Eastern Red	34	Pine, Longleaf
11	Cedar, Incense	35	Pine, Ponderosa
12	Cherry	36	Pine, Shortleaf
13	Cottonwood	37	Pine, Sugar
14	Cypress, Sapupira	38	Pine, White
15	Elm, American	39	Poplar, Yellow
16	Fir, Red	40	Ramin
17	Fir, White	41	Radiata Pine
18	Gum, Black	42	Redwood
19	Gum, Red	43	Spruce, Sitka
20	Hemlock, Western	44	SPF, COFI*
21	Hackberry	45	Teak
22	Hickory	46	Virola
23	Keruing	47	Walnut, Black
24	Larch	48	Western Hemlock - COFI*

SET TEMPERATURE

The J-2000 defaults to a temperature of 20°C. As wood temperature increases, its electrical resistance decreases and indicated moisture content rises. Lower wood temperatures result in lower indicated moisture content. A correction is necessary if the wood temperature is outside the range of 10°C to 32°C. Set the temperature accordingly and the meter will make the correction.

- **To change temperature** press and release the temperature button (#4). The meter will display the current temperature for one second.
- **To scroll forward** through the temperature settings, press and hold the temperature button (#4) while the current temperature is displayed.
- **To scroll backward** press and release the temperature button (#4). Within one second, press and hold the species button (#3). Continue to hold the species button (#3) and the temperature will decrease.
- **When scrolling in either direction**, release the button to stop at the desired temperature.

SET TEMPERATURE MODE

- **The meter will display the current temperature setting** and will wait one more second until shutting off so that you may change the temperature value as described above.

In Celsius, the temperature will change in increments of either 2°C or 3°C.

In the Celsius mode, positive values will display in whole numbers; negative values will display with a decimal point and a "-" sign in the left-hand corner. (i.e.: -17.0)

SET PIN CALIBRATION



The basic factory calibration of the J-2000 is for use with uninsulated pins – either the integral pins or with an optional external electrode, such as the #4-E.

The difference in readings between insulated and uninsulated pins is small below 10% moisture content. The difference increases as moisture content increases above 10%. When using an electrode with insulated pins, such as the 26-ES, you can change the calibration to compensate for this difference.

- **To change the pin setting**, press and release the species button (#3), then press the calibration check button (#2) within one second.
- **The meter will display** the current pin calibration as either 222 for insulated or 444 for uninsulated pins.
- **If you continue to hold the calibration check button (#2)** the meter will change pin calibration. The new calibration will remain in "memory" until you change it again, or you remove the battery.

TAKING A READING

The contact pins provided are best for stock up to 6/4. On stock over 6/4 or for hardwoods over 4/4 we recommend using a remote probe such as the 26-ES ram-type electrode. Mount the 26-ES directly to the external connector. See additional information under the "**Pin Talk**" section.

- **Remove the protective cover** to expose the pins. Check that the contact pins are firmly hand tightened.
- **To take a reading**, align the contact pins parallel to the grain and push them to their full penetration into the wood, if possible. Insulated pins read only at the tip and can be driven to the desired depth.
- **Press the read button (#1)** and read the moisture content on the meter scale. The meter displays the %MC for two seconds.
- **To add a reading to the sum** of all the previously stored readings, release the read button (#1) within 2 seconds.

INFORMATION ABOUT YOUR READINGS

Readings below 6% will be displayed as a numeric value, (-##.#), and will not be added to accumulation. A reading below 6% which is due to temperature and species adjustments will be shown as a numeric value with no minus sign and this reading will be added to the accumulation.

The meter will overrange at "40" The overrange indication is a blinking (40). Readings above 40% are not added to the accumulation

The meter will accumulate up to 100 readings. After all 100 readings are stored it will not add new readings until the memory has been cleared. It will also continue to display the average of all 100 readings as a reminder that the memory is full.

When taking and storing readings for a specific wood species, be sure to "clear" the meter before moving on to the next species if you do not want to group all of the readings together.

TO CHECK ACCUMULATED READINGS

This feature allows you to view the total number of all accumulated readings, the average of those readings, and the highest stored reading.

- **To view the readings** press and release the calibration check button (#2). First the meter displays the number of accumulated readings for one second, then the average of those readings for two seconds. Then it displays the highest stored reading for two seconds. The total "cycle" time is five seconds.
- **To erase readings** hold the calibration check button (#2) down for 5 seconds. All accumulated readings will be erased and the meter will display "0".

TO RESET METER

- **Press and release** the calibration check button (#2).
- **Within one second** press the species button (#3).
- **The meter will reset itself** and display in order "170" = #1 (Douglas Fir).

PIN TALK

There are two types of contact pins - uninsulated, which were provided with your meter, and insulated. When using uninsulated pins, push them in to the wood to their full length, if possible. This will give you the highest measured reading. Insulated pins read only at the tip and can be driven to a desired depth to gather shell and core (gradient) information. Additional types and lengths of both the insulated and uninsulated pins are available for specific applications.

CARE OF YOUR METER

To keep your meter in good working order:

- ✓ Store your meter in a clean, dry place. The protective carrying case provided is an ideal storage place when the meter is not in use.
- ✓ Change the 9-Volt battery as needed. Continued use with a low battery may cause the meter to go out of calibration.
- ✓ Change contact pins as needed. Keep pin retainers hand tightened.
- ✓ Clean the meter, contact pins, and probes with any biodegradable cleaner.
- ✓ Use the cleaner sparingly and on external parts only. Keep the cleaner out of the external connector.
- ✓ DO NOT IMMERSER THE METER OR ANY ELECTRODE IN WATER.
- ✓ Remove the battery if the meter will not be used for one month or longer.

SERVICE FOR YOUR METER

- ✓ Pack your meter securely. Enclose a purchase order or letter with a brief description of the problem.
- ✓ There is no need to call us for a return authorization number if you are within the EU. Customers outside the EU must contact us for more specific instructions prior to returning a meter.
- ✓ Include your name, address, daytime phone and fax numbers or e-mail address. If you believe the meter is under warranty, please provide the original sales slip or invoice.
- ✓ Ship via UPS, Express Mail, Priority Mail or any overnight courier who provides prompt service. Do not use standard parcel post.
- ✓ Insure your instrument for its full value and ship prepaid. We are not responsible for damage in transit.
- ✓ We do not accept COD shipments or cover any incoming freight or duty charges on returned merchandise
- ✓ Turnaround time on repairs is approximately two weeks.
- ✓ We will call you with an estimate if you specifically request one, or if we determine that the meter may be too costly to repair.
- ✓ Non-warranty repairs will be returned via UPS/COD unless you have already established other payment terms. There is no COD service outside the EU.
- ✓ Payments have to be made by Bank transfer prior to the return shipment. A proforma invoice will be raised in advance.
- ✓ Warranty repairs will be returned at no charge if shipped within the EU via UPS Ground Service. Freight charges for expedited services (i.e., Federal Express, UPS/2 Day, UPS/1 Day, etc.) are the customer's responsibility and will be charged as per the above terms.

WARRANTY

Delmhorst Europe, referred to hereafter as Delmhorst, guarantees your moisture meter for one year from date of purchase and any optional electrodes against defects in material or workmanship for 90 days. If, within the warranty period of the meter, you find any defect in material or workmanship return the meter following the instructions in the "**Service for Your Meter**" section. This limited warranty does not cover abuse, alteration, misuse, damage during shipment, improper service, unauthorized or unreasonable use of the meter or electrodes. This warranty does not cover batteries, pin assemblies, or pins. If the meter or any optional electrodes have been tampered with, the warranty shall be void. At our option we may replace or repair the meter. Delmhorst shall not be liable for incidental or consequential damages for the breach of any express or implied warranty with respect to this product or its calibration. With proper care and maintenance the meter should stay in calibration; follow the instructions in the "**Care of Your Meter**" section.

Under no circumstances shall Delmhorst be liable for any incidental, indirect, special, or consequential damages of any type whatsoever, including, but not limited to, lost profits or downtime arising out of or related in any respect to the meters or electrodes and no other warranty, written, oral or implied applies. Delmhorst shall in no event be liable for any breach of warranty or defect in this product that exceeds the amount of purchase of this product. The express warranty set forth above constitutes the entire warranty with respect to Delmhorst meters and electrodes and no other warranty, written, oral, or implied applies. This warranty is personal to the customer purchasing the product and is not transferable.

ARTTEST B.V.
Tradenname DELMHORST EUROPE
TITANIUMLAAN 100
NL 5221 CK 's-HERTOGENBOSCH
THE NETHERLANDS
info@delmhorst.eu
www.MoistureMetersDelmhorst.com
+31 (0)73 6395080

For over 65 years, Delmhorst is a leading brand for high-quality resistance moisture meters. Today the Delmhorst range consists of a complete line of portable moisture meters for a variety of different applications including woodworking / lumber, agriculture, construction and paper.

DECLARATION OF CONFORMITY

Manufacturer's Name: Delmhorst Instrument Co.

Manufacturer's Address: 51 Indian Lane East
Towaco, NJ 07082
USA

Council Directive(s): 89/336/EEC - Meets EMC directive
73/23/EEC - Not required. Voltage used or generated
is not within scope of Low Voltage Directive.


Standard(s) to which Conformity is declared :

EN 50082-1:1992- EMC Generic immunity standard
EN 50081-1:1992- EMC Generic emission standard
EN 55011:1991- Limits and methods of measurement of
radio disturbance characteristics of (ISM) equipment.

Type of Product : Wood Moisture Meter

Model No. J-2000/X

I, the undersigned, hereby declare that the product specified above conforms to the above Directive(s) and Standard(s).

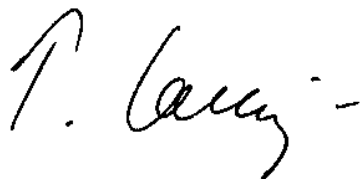

Thomas Laurenzi, President
Delmhorst Instrument Co.
NJ, USA